





# *Talos*™



Thoracic Stent Graft System

The Dissection Specific Stent Graft

**Proximal rounded bare stent**  
Reduces the stress on stent apices

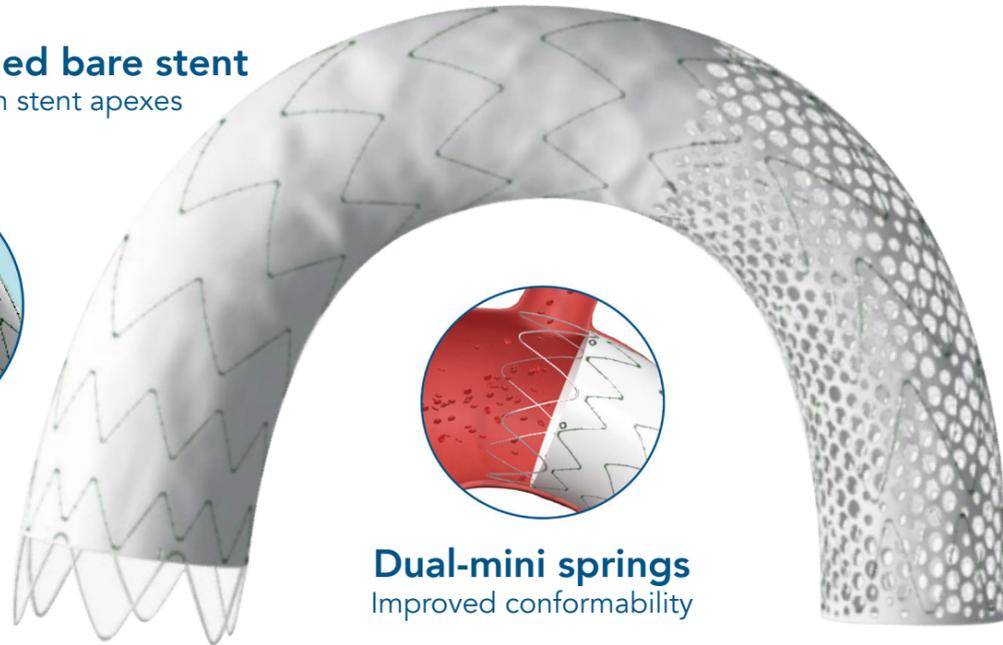

**Dual-mini springs**  
Improved conformability

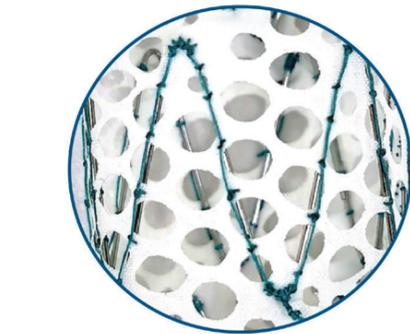


**Distal Honeycomb Design**

**Avoids the risk of paraplegia preserving the supply of the intercostal artery while remodelling the distal true lumen**


**0%** Paraplegia at 12 months

\* from the Talos pre-market clinical trial. Data on file MicroPort Endovastec


**Tip capture mechanism**



**Low-Profile delivery system**  
20F and 22F

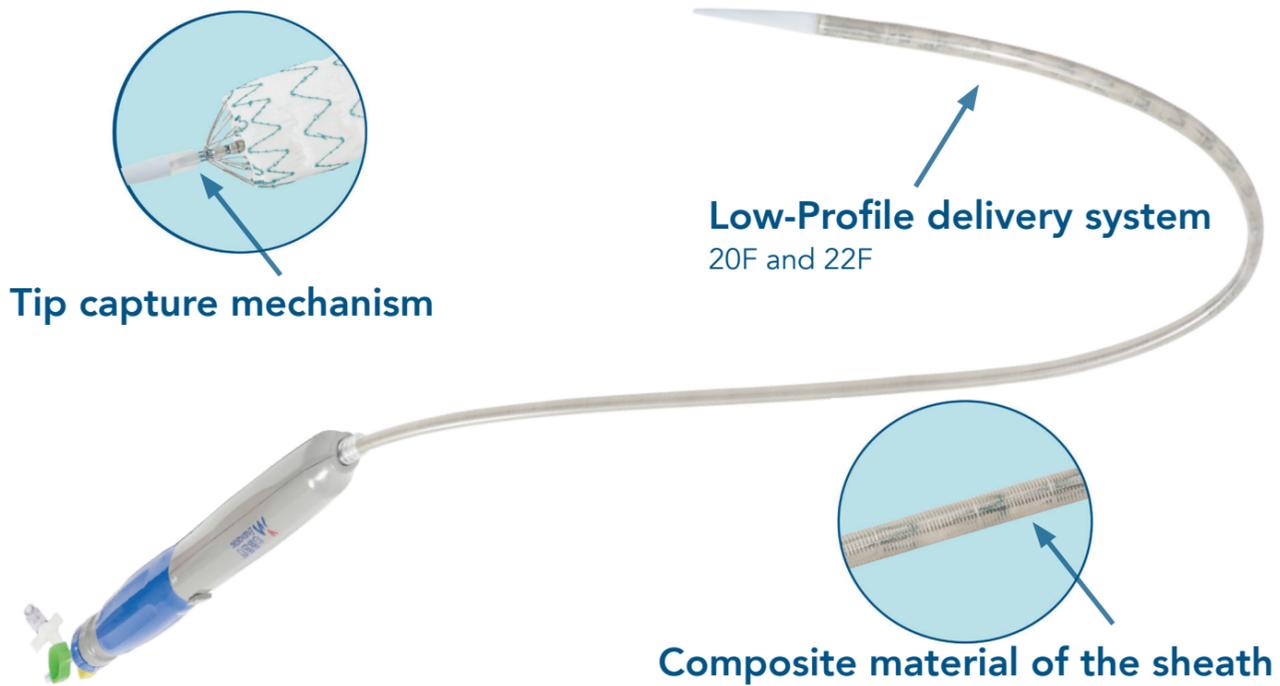


**Composite material of the sheath**  
High Flexibility




**Retract the outer sheath**  
Push up the rotation lock and rotate the handle in a clockwise motion



**Deploy the stent-graft**  
Rotate the rotation handle clockwise to label 1 and pull the yellow ring




**Tip capture mechanism**  
Rotate the handle clockwise to label 2 and pull the green ring




# Model Specifications

## Talos™ Thoracic Stent-Graft

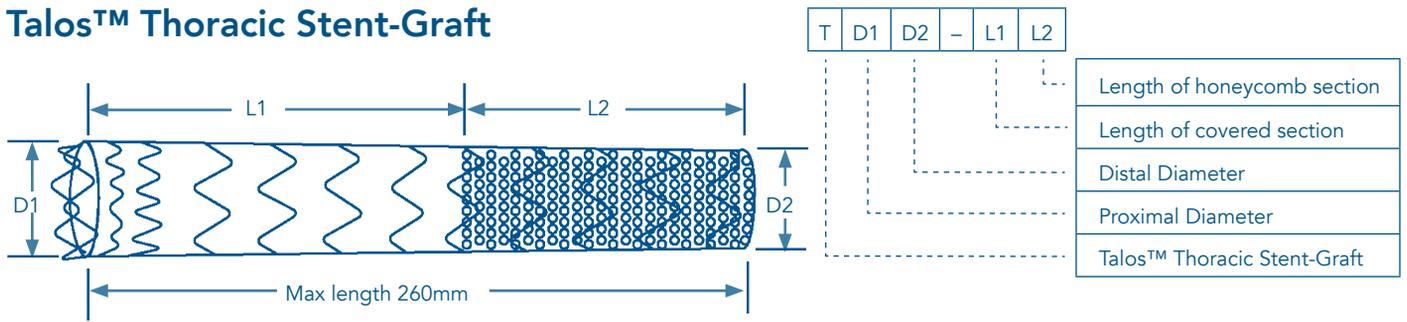

Size Description	Size Range (mm)
Proximal Diameter (D1)	26 / 28 / 30 / 32 / 34 / 36 / 38 / 40
Distal Diameter (D2)	20 / 22 / 24 / 26 / 28 / 30 / 32 / 34
Length of covered section (L1)	100 / 160 / 200
Length of honeycomb section (L2)	60 / 100
Tapering Options	4 / 6

## Talos™ Honeycomb Extension

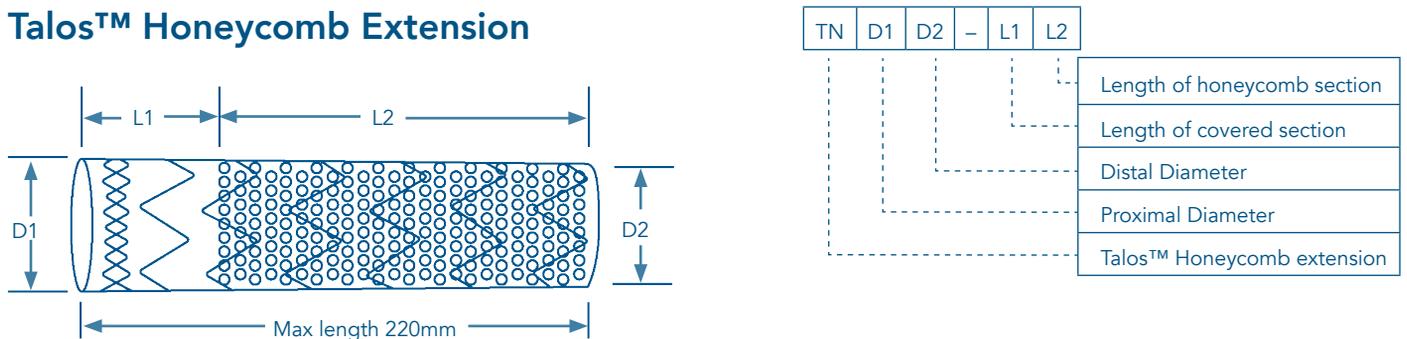

Size Description	Size Range (mm)
Proximal Diameter (D1)	28 / 30 / 32 / 34 / 36 / 40
Distal Diameter (D2)	22 / 24 / 26 / 28 / 30 / 32 / 34 / 36 / 38 / 40
Covered stent graft (L1)	20
Honeycomb section (L2)	100 / 140 / 180
Tapering Options	0 / 4 / 6

Contact your local Sales Representative to confirm the feasibility of the requested design



Lombard Medical Limited, Lombard Medical House, 4 Trident Park, Didcot, OX11 7HJ  
 Tel: +44 (0)1235 750800 Email: globalinfo@lombardmedical.com Website: www.lombardmedical.com

All cited trademarks are the property of their respective owners in respective countries. These devices should only be used by a licenced physician. Indicators, contraindications, warnings, potential adverse events and directions for use can be found in Instructions for Use and product labelling supplied with each device. The promotion, distribution or sale of these devices is prohibited in countries where the registration certificates or any other licences have not been obtained. This brochure is for the use of the individuals to whom it has been provided and is not to be distributed widely as an advertisement. Any information may be changed without prior notice. Talos™ is manufactured by MicroPort Endovastec and Distributed in Europe by Lombard Medical Limited. Not Available for sale in the United States.  
 ©2025 Lombard Medical Limited. All rights reserved. D01485\_ENG A